

FIG. 1
Prior Art

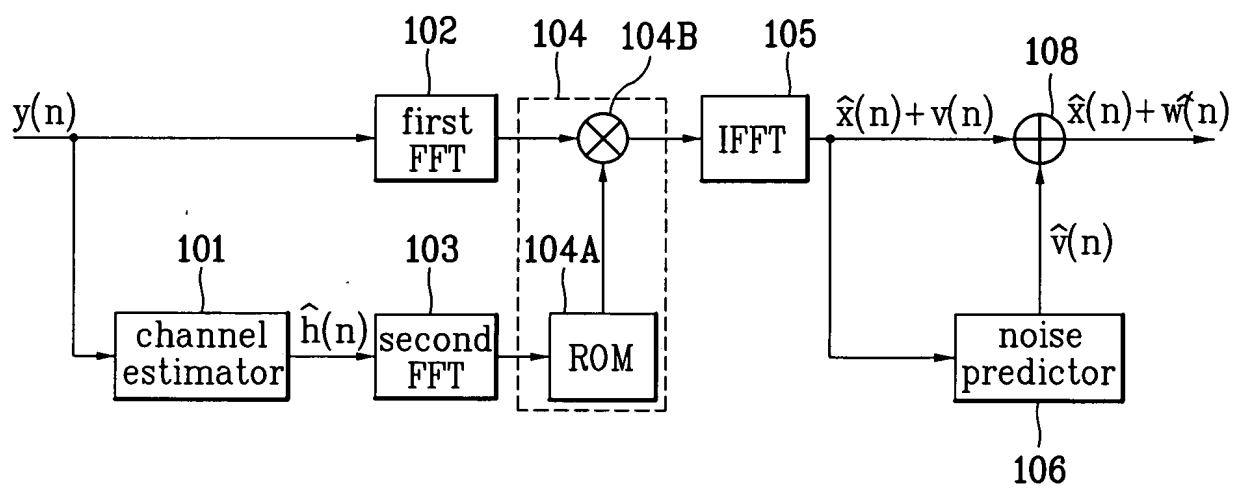


FIG. 2

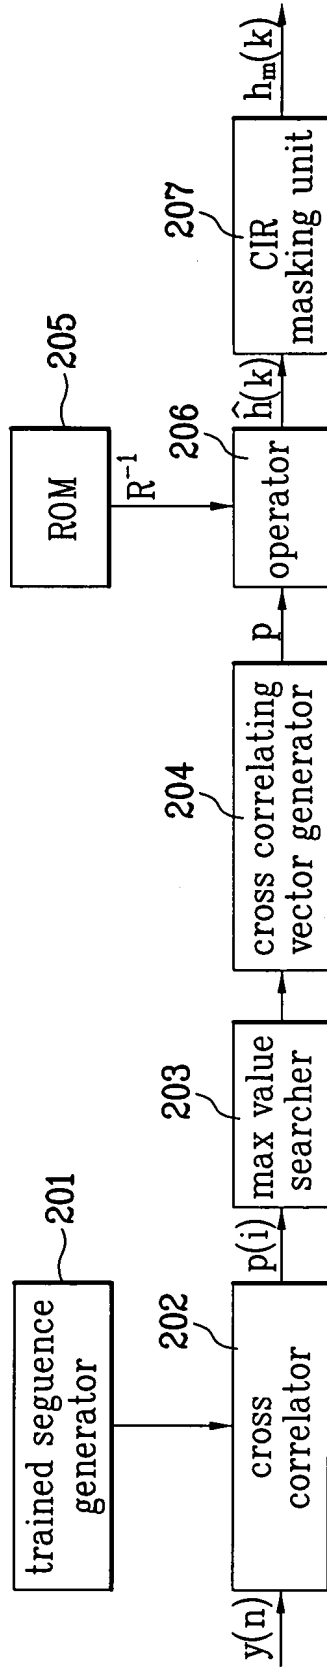


FIG. 3

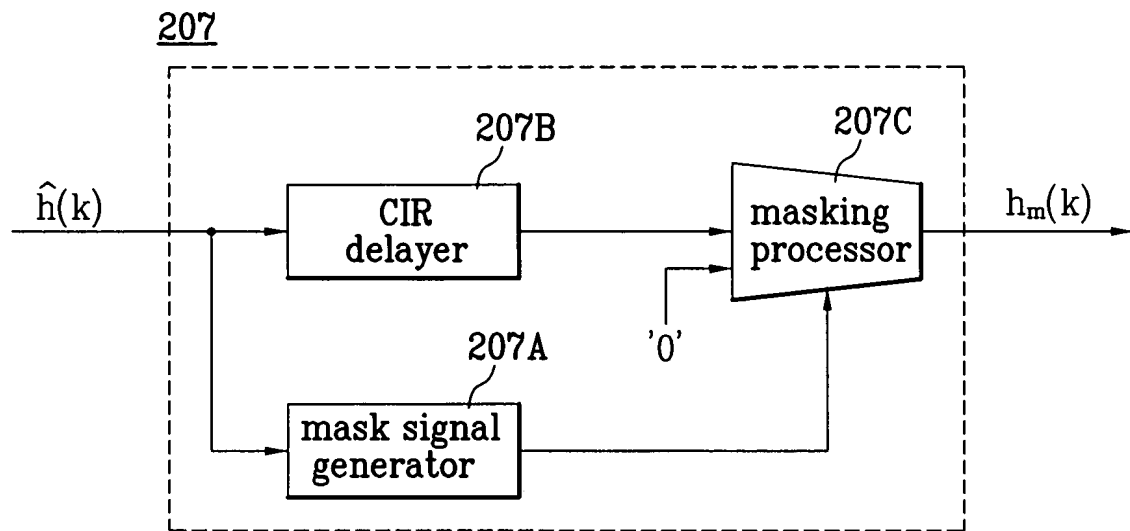


FIG. 4A

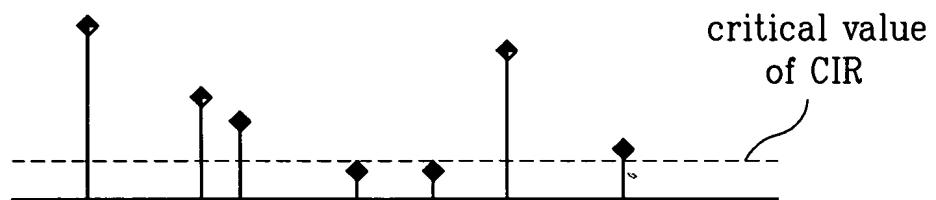


FIG. 4B



FIG. 4C

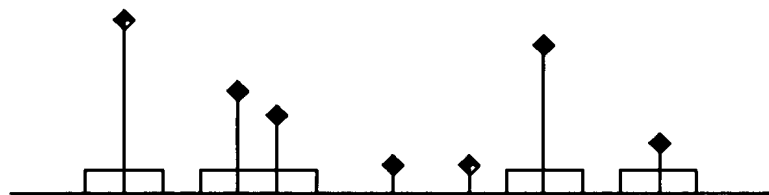


FIG. 4D

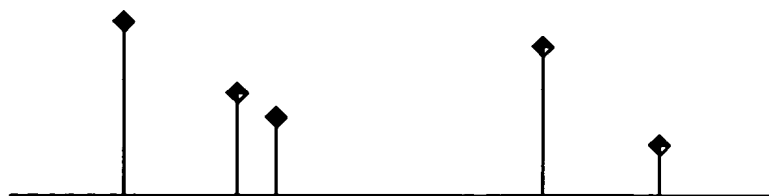


FIG. 5A

		Raw CIR	Masked CIR
measurement times of time average.	0	X	26.7dB
	2	17.3dB	
	4	20.3dB	
	8	22.5dB	

FIG. 5B

		Raw CIR	Masked CIR
measurement times of time average.	0	X	22.7dB
	2	X	
	4	X	
	8	20.2dB	

FIG. 5C

		Raw CIR	Masked CIR
measurement times of time average.	0	X	21.5dB
	2	X	
	4	X	
	8	X	